

CERAMENT® G






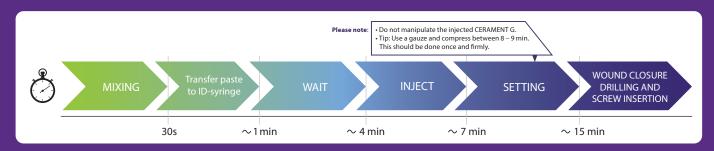

- Draw air into the syringe up to the red line.
- Attach the vial to the syringe.
- Plunge all the air into the vial.



- Withdraw liquid up to the red mark on the syringe. There should be saline left in the vial.
- Disconnect the rotating adapter and vial from the syringe.




a) Attach the syringe to the spike.b) Inject <u>all</u> solution into the vial.




• Dissolve all the gentamicin powder.



 Withdraw <u>all</u> the gentamicin solution back into the syringe. This may require the spike to be slightly backed out.




 Retract the blue handle and remove the red plunger stop ring.

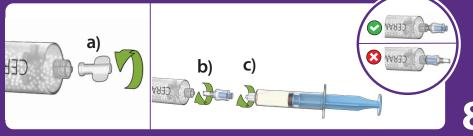


- b) Attach valve, clear end to the powder filled syringe, and turn clockwise.
- c) Attach syringe with gentamicin solution to blue end of valve, press and turn clockwise.




- Inject all the gentamicin solution into the syringe with powder.
- Keep the plunger pushed to the bottom to avoid back flush.
- Detach the syringe from the valve.



- After the liquid has been injected, start the stopwatch immediately.
- Mix with rotation for 30 seconds, at 1 complete stroke per second.
- Push the handle all the way down and pull it all the way up, and rotate at its end positions.



- a) Fully retract blue handle.
- b) Lock plunger by turning blue collar clockwise to click.



- a) Attach dispensing syringe to valve.
- b) Transfer paste with numbers facing user. When full, paste will begin to ooze from under sleeve. Stop filling when this occurs.



 Do not remove the red stopper until ready to inject.







bonesupport.com
PR 1077-02 en AU CA EU ROW 01-2022